



Change of bilateral difference in radial artery pulse morphology with one-side arm movement



Xinge Jiang ^{a,b}, Shoushui Wei ^{a,**}, Dingchang Zheng ^c,
Feifei Liu ^a, Shouqin Zhang ^b, Zhimin Zhang ^a, Chengyu Liu ^{a,*}

^a School of Control Science and Engineering, Shandong University, Jinan 250061, China

^b Shandong College of Electronic Technology, Jinan 250200, China

^c Health & Well Being Academy, Faculty of Medical Science, Anglia Ruskin University, Chelmsford CM1 1SQ, UK

Received 9 February 2017; received in revised form 4 April 2017; accepted 26 April 2017

KEYWORDS

Arterial volume compliance;
Artery pulse;
Radial artery pulse

Abstract Previous studies have demonstrated that the compliance of peripheral artery changes with arm movement. This study aimed to quantify the bilateral difference in radial artery pulse morphology with one-side arm movement. Twenty-four healthy subjects were recruited. Radial artery pulses were synchronously recorded from both arms, with one arm (left or right) at five different positions (90°, 45°, 0°, −45° and −90°) and the other arm at horizontal level (0°) as reference. Two types of indices of arterial pulse morphology were derived from the normalized arterial pulse signals: the waveform width corresponding to the 50%, 60% and 70% pulse amplitude (W_{50} , W_{60} , W_{70}) and the total area of normalized pulse waveform (A_{pulse}). No matter whether the moving arm was left or right arm, when compared with the other side reference arm, all the waveform widths decreased with arm moving from 90°, 45°, 0°, −45°, and −90°. The bilateral difference of W_{50} , W_{60} and W_{70} with the moving arm (either left or right) at 90°, 45° were significantly positive (both $p < 0.01$) and significantly negative at −90° (both $p < 0.05$). Meanwhile, no matter whether the moving arm is left or right, A_{pulse} decreased with arm moving from 90°, 45°, 0°, −45°, and −90°. The bilateral difference of A_{pulse} with the left moving arm were significantly positive at 45°, 90° (both $p < 0.05$). Meanwhile, the bilateral difference of A_{pulse} from the moving right arm was significantly positive at 90° and significantly negative at −45° and −90° (all $p < 0.05$). In summary, this study quantified the bilateral arterial pulse morphology between arteries with different compliances induced by a simple arm positioning procedure.

© 2017 Association for Research into Arterial Structure and Physiology. Published by Elsevier B.V. All rights reserved.

* Corresponding author.

** Corresponding author.

E-mail addresses: sswei@sdu.edu.cn (S. Wei), bestlcy@sdu.edu.cn (C. Liu).

Introduction

Arteries play an important role in cardiovascular physiology and pathophysiology. Arterial properties can change with different physiological and clinical conditions,^{1–4} including aging,^{5,6} hypertension,³ diabetes,⁴ heart failure^{1,7} drug treatment,⁸ smoking,⁹ alcohol¹⁰ and emotion states.¹¹ It is clinically important to characterize and quantify the elastic properties of arteries. Various non-invasive techniques have been used to indirectly quantify the properties of arteries. The most commonly used technique measures pulse wave velocity (PWV) or pulse transit time (PTT).^{12–14} Analysis of pulse waveform shape characteristics has also been accepted as another non-invasive technique. The difference in finger pulse amplitude changes with changing pressure have been explored in patients with cardiovascular diseases.¹⁵ The carotid waveform morphology has also been used to investigate the difference between the peripheral and central arterial pressure pulses.¹⁶

Recently, Zheng and Murray^{12,17} reported a simple technique through arm moving to induce the change of peripheral arterial volume distensibility and concluded that the peripheral arteries are more compliant with the arm positioned above horizontal level in comparison with the arm at the horizontal level.¹⁸ To the best of our knowledge, the arterial pulse morphology change with arm moving has not been quantified. Therefore, the first aim of this study was to quantify the radial pulse morphology changes for arteries with different compliances induced by positioning the arm at different positions. For healthy subjects, the bilateral radial pulse morphology should be almost the same if both arms are positioned at the same height levels. By positioning one arm at horizontal level as reference and the other arm at a different height, a bilateral pulse morphology difference could be introduced, and its changes with arm positions could be quantified. Thus, the bilateral pulse morphology difference from the synchronously recorded bilateral radial pulses, i.e., between the moving arm (at five different positions 90°, 45°, 0°, –45°, and –90° to the horizontal level) and the reference arm (at horizontal position 0°), would be quantified.

Methods

Subjects

Twenty-four healthy subjects (14 male and 10 female) aged between 21 and 50 were enrolled in this study. Their basic clinical information is presented in Table 1. The study received ethical permission from the local Ethical Committee of Shandong University in China, and all subjects gave their written informed consent to participate in this study.

Arterial pulse recording procedure

All the measurements were undertaken in a quiet room at Shandong University. Each subject was asked to lie down on a measurement bed for 5 min before the formal arterial pulse recording to allow cardiovascular stabilization. All the measurements were operated by the same operator.

Table 1 Basic clinical information for the 24 subjects studied.

Variables	Value	Range (min–max)
Number (M/F)	24 (14/10)	—
Age (year)	29 ± 8	21–50
Height ¹⁹	169 ± 8	151–183
Weight (kg)	63 ± 11	41–87
BMI (kg/m ²)	22 ± 3	15–27
SBP (mmHg)	115 ± 12	93–137
DBP (mmHg)	70 ± 10	57–95
MAP (mmHg)	85 ± 10	69–107

Value is expressed as number (male/female) or mean ± standard deviation (SD). BMI: body mass index, SBP: systolic blood pressure, DBP: diastolic blood pressure, MAP: mean arterial pressure.

For each subject, there were two repeat measurement sessions with an interval of 20 min. Within each measurement session, two series of five separate recordings were performed with one arm at five different positions (90°, 45°, 0°, –45°, and –90° to the horizontal level) and the other arm at horizontal position (0°) as the reference arm, and then vice versa, i.e., firstly, the right arm was regarded as the ‘moving arm’ by positioning at five positions and the left arm as the ‘reference arm’; then the left arm was regarded as the ‘moving arm’ with recordings at five positions and the right arm as the ‘reference arm’. Figure 1(A) shows the schematic diagram of the measurement procedure and a picture of the set-up. In total, 20 arterial pulse recordings were obtained from each subject (from 2 repeat session, 5 recordings with the left arm as moving arm and 5 recordings with the right arm as the moving arm).

During each recording, all subjects remained supine position on a measurement bed. Piezoelectric sensors (manufactured by Hefei-Huake Electronic Technology Research Institute, China) were placed in the radial arteries of both arms and were fixed using two same size bandages (as shown in Fig. 1(B)). When arterial pulse signals were stably and clearly shown on the display screen, the moving arm was positioned at the measurement height by a mechanical support to avoid the movement and the reference arm was constantly kept at horizontal position. The radial artery pulses from both two side arms were simultaneously recorded for 40 s with a sampling rate of 500 Hz.

At the beginning and end of each study, systolic and diastolic blood pressures (SBP and DBP) were measured using a clinically validated BP monitor (102, Dongyue healthcare, Shandong, China) with both arms at the horizontal level. Mean arterial pressure (MAP) was calculated used the equation: $MAP = DBP + 0.4(SBP - DBP)$.²⁰

Arterial pulse processing

For each recording, the feet of the recorded radial artery pulses were detected by an open-source algorithm^{21,22} and then manually verified. 11 consecutive stable and high




Figure 1 (A) The schematic diagram of the measurement procedure with the right arm (moving arm) at different positions and the left arm was regarded as 'reference arm'. (B) the Piezoelectric sensors were placed in the radial arteries of both arms and were fixed using two same size bandages.

quality beats were chosen by manual. Then 11 separate beats were extracted respectively between two adjacent pulse feet. In order to eliminate the effects of changes in appplanation pressure, the pulse waveform is normalized. Each beat was then normalized with the length of 1000 points and amplitude of 1 (i.e., pulse foot had amplitude of 0 and pulse peak of 1). Normalized mean pulse template (NMPT) was then constructed by averaging 11 normalized pulses from each recording. Figure 2 shows the examples of five NMPTs with the left arm at 90°, 45°, 0°, -45° to -90° to the horizontal level. For each subject, a total of 40 NMPTs are obtained, with 20 NMPTs from the moving arm (left or right) at the five different positions (2 repeat sessions, 2 moving arms, 5 positions), as well as 20 NMPTs from the reference arm.

Pulse morphology indices and their bilateral differences

To quantify the pulse morphology changes with the arm at different positions, two types of indices were defined. One was the pulse waveform width index, which was defined as a pulse waveform width corresponding to a certain percentage of the pulse amplitude. In this study, three pulse waveform width indices (W_{50} , W_{60} and W_{70}) corresponding to 50%, 60% and 70% of pulse amplitude were considered. Another index was the total area of the NMPT signal (A_{pulse}). Figure 3 demonstrates their definitions.

The bilateral waveform width difference and the bilateral total area difference were then calculated between the moving arm (at five different positions 90°, 45°, 0°, -45°, and -90° to the horizontal level) and the corresponding reference arm (at horizontal position 0°) to obtain the bilateral pulse morphology differences.

Data and statistical analysis

The mean and SD values of the obtained indices (A_{pulse} , W_{50} – W_{70} , and their bilateral differences) were firstly calculated, separately for each arm at different positions. The effect of arm position on the bilateral pulse morphology differences was then tested. A $p < 0.05$ was considered statistically significant.

Results

Changes of bilateral difference of W_{60} with arm moving

Our results show that the changes of W_{50} , W_{60} and W_{70} with arm moving were similar and there was no significant difference between these three indices at different arm positions. To simplify the results, W_{60} was used to describe the results in details.

Figure 4(A) and (B) shows overall means and their SDs of index W_{60} with the moving arm (left or right) at different positions (90°, 45°, 0°, -45°, and -90°) and the other arm at horizontal level as reference. Whether left arm or right arm, W_{60} decreased with arm moving from 90°, 45°, 0°, -45°, and -90°. When compared with the reference arm, W_{60} from the moving left arm were significantly larger at 90°, 45° (both $p < 0.01$) and significantly smaller at 0°, -90° (both $p < 0.05$), while not at -45°. Meanwhile, W_{60} from the moving right arm were significantly larger at 90°, 45° (both $p < 0.01$) and significantly smaller at -90° ($p < 0.05$), while not at 0° and -45°. As shown in Fig. 4(C) and (D), for left arm moving, the mean bilateral W_{60} differences were 54.9, 34.1, 8.6, -4.2 and -9.0 respectively for the five positions, and for right arm moving, their corresponding mean differences were 53.1, 35.4, 2.1, -5.9 and -11.2 respectively.

Changes of bilateral difference of A_{pulse} with arm moving

Figure 5(A) and (B) shows overall means and their SDs of index A_{pulse} with the moving arm (left or right) at different positions (90°, 45°, 0°, -45°, and -90°) and the other arm at horizontal level as reference. Whether left arm or right arm, A_{pulse} decreased with arm moving from 90°, 45°, 0°, -45°, and -90°. When compared with the reference arm, A_{pulse} from the moving left arm were significantly larger at 90° ($p < 0.01$) and 45° ($p < 0.05$), while not at 0°, -45° and -90°. Meanwhile, A_{pulse} from the moving right arm was significantly larger at 90°, and significantly smaller -45° and -90° (both $p < 0.05$), while

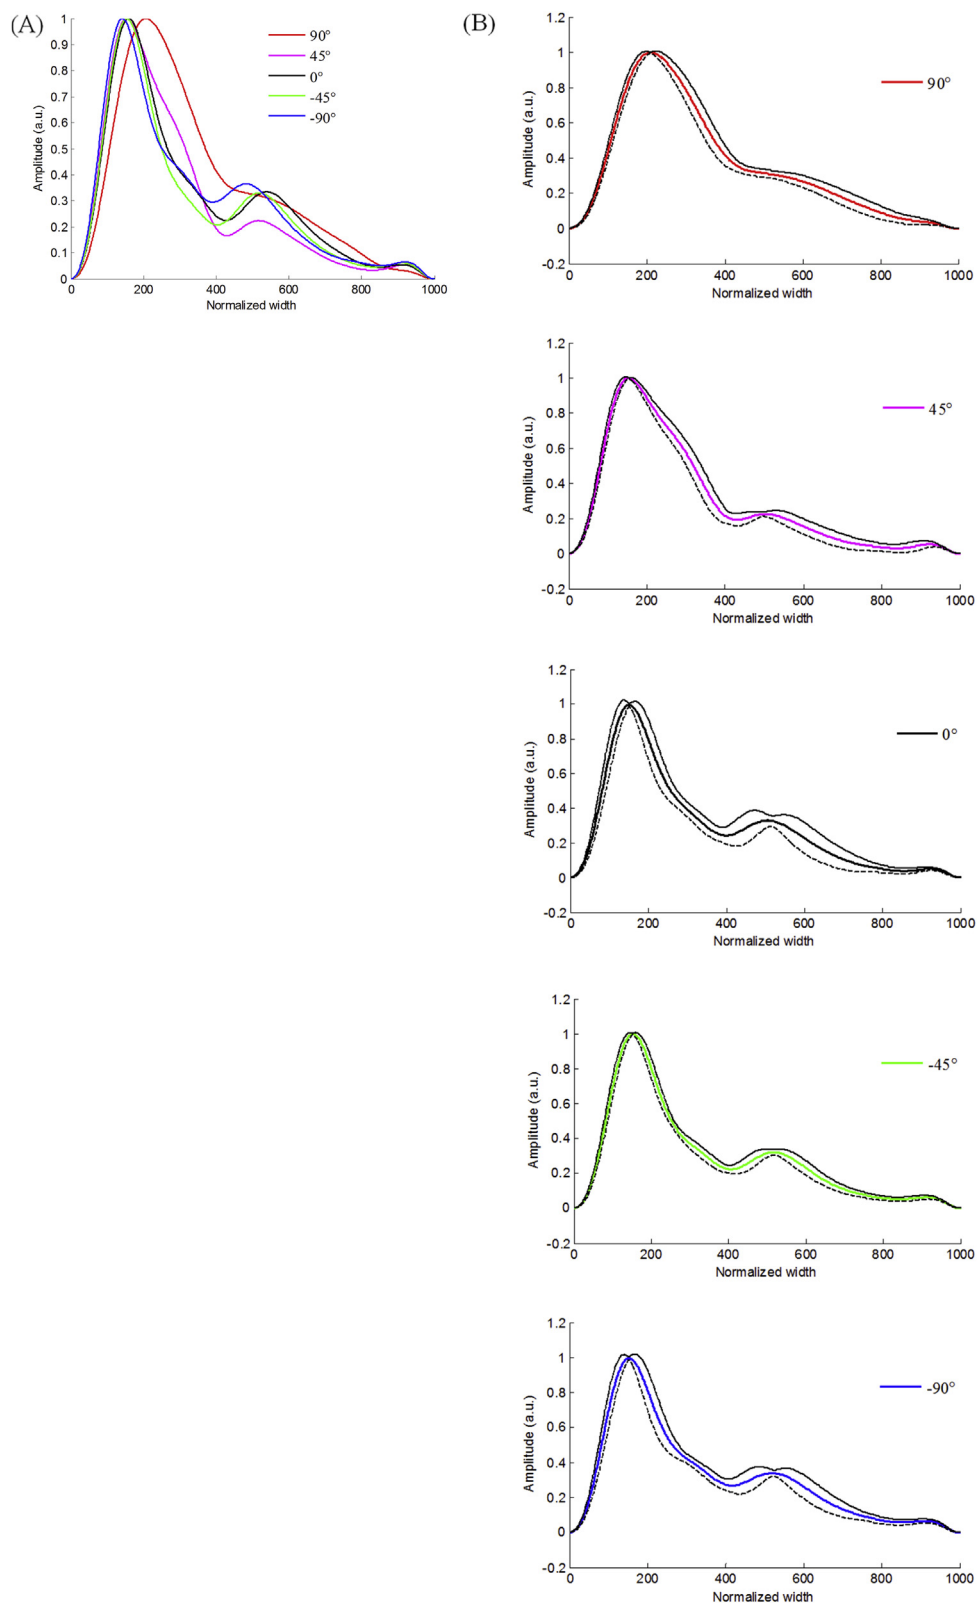


Figure 2 Examples of five NMPTs from one subject with the left arm at five different positions (90°, 45°, 0°, -45°, and -90° to the horizontal level). (A) show the five mean NMPTs and (B) shows the detailed three curves (average curve (thick solid line) and the mean \pm 2 SDs curves (thin solid and dotted lines respectively)) for each position.




Figure 3 Definitions of the two indices: pulse waveform width (W_{60} as an example) and area of pulse waveform (A_{pulse}).

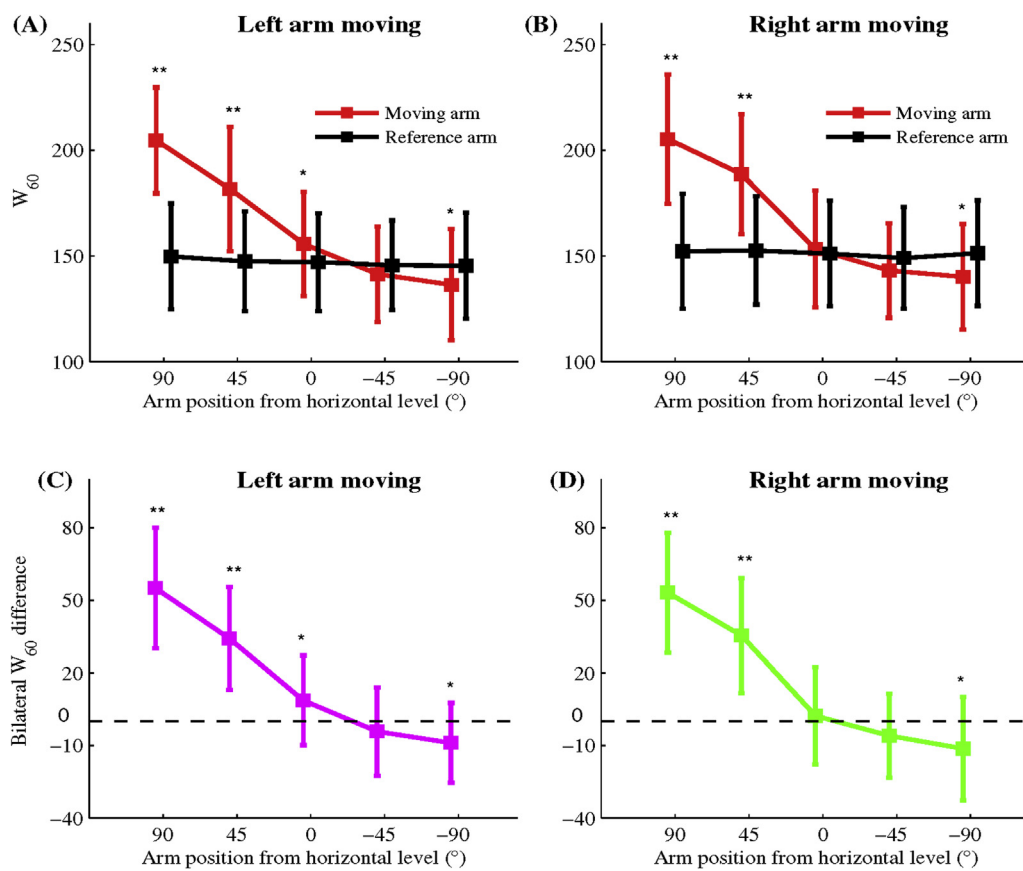


Figure 4 Results of index W_{60} with the moving arm (A and C for left arm, and B and D for right arm) at five different positions (90°, 45°, 0°, -45°, and -90° to the horizontal level) and the other side arm at horizontal level as reference: (A) and (B) show the means and standard deviations (SDs) for index W_{60} respectively, and (C) and (D) show the bilateral W_{60} difference between the moving arm and the reference arm, with the dotted zero line. * means significant statistical difference for $p < 0.05$ and ** means significant statistical difference for $p < 0.01$.

not at 45° and 0°. As shown in Fig. 5(C) and (D), for left arm moving, the mean bilateral A_{pulse} differences were 30.3, 11.1, 6.3, -8.1 and -7.0 respectively for the five positions, and for right arm moving, the corresponding mean differences were 19, 4, -4, -14 and -13 respectively.

Discussion

This study quantified the bilateral radial artery pulse shape difference between the moving arm (at five different positions 90°, 45°, 0°, -45°, and -90° to the horizontal level) and the reference arm (at horizontal position 0°). These

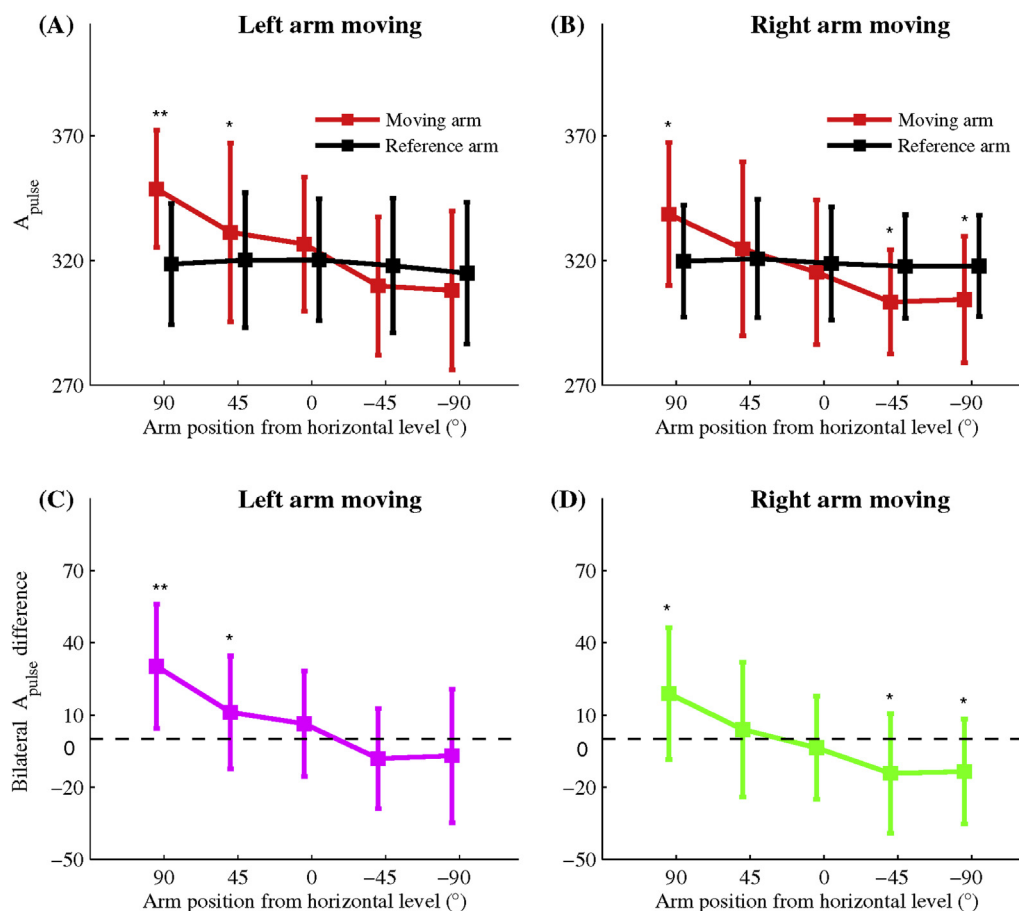


Figure 5 Results of index A_{pulse} with the moving arm (A and C for left arm, and B and D for right arm) at five different positions (90°, 45°, 0°, -45°, and -90° to the horizontal level) and the other side arm at horizontal level as reference: (A) and (B) show the means and standard deviations (SDs) for index A_{pulse} respectively, and (C) and (D) show the bilateral A_{pulse} difference between the moving arm and the reference arm, with the dotted zero line. * means significant statistical difference for $p < 0.05$ and ** means significant statistical difference for $p < 0.01$.

changes were quantified by two indices (pulse waveform width and normalized pulse area). Specifically, bilateral W_{40} , W_{50} , W_{60} and A_{pulse} difference were quantified, which decreased gradually and significantly with the arm moving from 90° to 45°, 0°, -45°, and -90° respectively.

The effect of arm position on heart rate has been counted in this paper. The means and SDs of heart rate with arm moving from 90°, 45°, 0°, -45°, and -90° were 66.6 ± 5.1 , 66.9 ± 5.5 , 66.8 ± 5.2 , 66.9 ± 5.2 and 67.1 ± 5.0 beat/min respectively. Our results were consistent with results of previous research that the subject's heart rate did not change if the subject kept quiet, whether supine or sitting, with the arm passively positioned in different positions by a support, in a way that the arm kept relaxed without muscle tension.^{23,24}

The changes of elastic properties of arteries are associated with different physiological and clinical conditions induced by the change of BP. Previous studies have found important differences between indirect BP readings when the arm was placed in different positions.^{23,25,26} Both SBP and DBP values were significantly decrease when the arm were elevated above the level of the right atrium, while significantly increase when lowered below the level of the right atrium. Previous studies also studied the influence of

body posture on the indirectly measured BP values when the arm was placed at the right atrium level and showed that both SBP and DBP were significantly higher in the supine than those in the sitting position.²⁷ In our current study, all subjects were asked to keep a supine position and both arms were constantly kept at heart level at 0° measurement.

With elevating the arm, the effect of gravity induces a hydrostatic pressure difference. Mitchell et al.²⁸ and Netea et al.²⁶ reported that the change of BP values taken from the arm at different levels versus the reference level of the right atrium could almost completely be explained by the effect of hydrostatic forces. The change of BP affects the arterial compliance. Pucci et al. researched the relationship between the arterial compliance and BP with the arm movement, and reported that, relative to the heart level, radial augmentation index increased with the arm elevating and decreased with the arm reducing.²³

Zheng and Murray¹⁸ reported that the peripheral arteries compliant with the arm positioned above horizontal level in comparison with the arm positioned below horizontal level by measuring PTT difference. However, this conclusion was from the unilateral finger/ear PPG measurements, not from the simultaneously recorded bilateral radial artery

measurements as in this study. Different from the published study by Zheng et al., two pulse waveform morphology indices, i.e., W_{60} and A_{pulse} , were used in the current study, and the effect of arm position on arterial pulse waveform was investigated from simultaneously recorded bilateral radial pulse waveforms, avoiding the potential physiological variations with time.

Previous studies assessed the change of elastic properties by measuring PWV, but produced different clinical conclusions, with no change,²⁹ higher^{19,30} and lower³¹ of PWV results. These conflicting results may be partly due to the different segments of arteries used for investigation or/and the methodological difference. Further investigation on pulse morphology is therefore worthwhile.

If the peripheral arterial system had relatively higher compliance, a larger proportion of the ejected blood would expand the peripheral arteries and hence the radial artery pulse would be expected to have bigger pulse's area and width of pulse waveform.⁵ In the current study, it has been observed both pulse waveform's width and area indices increased with arm raising, where the arteries are more compliant. Therefore, our results agreed with the published expectation and demonstrated that the change of pulse waveform's width and area indices could be used to quantify the change of arterial compliance with a simple arm positioning procedure.

As the comparison of the two indices W_{60} and A_{pulse} , it is observed that W_{60} was better than A_{pulse} in response to arterial compliance changes since the effect of arm position on W_{60} was larger as shown in Figs. 4 and 5. In addition, from Figs. 4 and 5, slight difference was observed between the left and right arms at 0° level. This result may be partly due to the physiological structure difference of the left and right arms.

In conclusion, this study quantified the bilateral difference of the two pulse morphology indices, i.e., W_{60} and A_{pulse} , with the arm at different positions, which indicated that these indices could be potentially used for quantifying arterial compliance changes.

Conflict of interest statement

The authors declare no conflict of interest.

Acknowledgments

This research was sponsored by the National Natural Science Foundation of China (grants 61671275 and 61201049) and the Natural Science Foundation of Shandong Province in China (grant 2014ZRE2733).

References

- Liu CY, Zheng DC, Zhao LN, Li P, Li B, Murray A, et al. Elastic properties of peripheral arteries in heart failure patients in comparison with normal subjects. *J Physiol Sci* 2013;63:195–201.
- Joyner MJ. Effect of exercise on arterial compliance. *Circulation* 2000;102:1214–5.
- Arnett DK, Boland LL, Evans GW, Riley W, Barnes R, Tyroler HA, et al. Hypertension and arterial stiffness: the atherosclerosis risk in communities study. *Am J Hypertens* 2000;13:317–23.
- Benetos A, Waeber B, Izzo J, Mitchell G, Resnick L, Asmar R, et al. Influence of age, risk factors, and cardiovascular and renal disease on arterial stiffness: clinical applications. *Am J Hypertens* 2002;15:1101–8.
- Liu CY, Zheng DC, Murray A. Arteries stiffen with age, but can retain an ability to become more elastic with applied external cuff pressure. *Medicine* 2015;94:e1831.
- Allen J, Oates CP, Lees TA, Murray A. Photoplethysmography detection of lower limb peripheral arterial occlusive disease: a comparison of pulse timing, amplitude and shape characteristics. *Physiol Meas* 2005;26:811–21.
- Liu CY, Zheng DC, Zhao LN, Liu CC. Gaussian fitting for carotid and radial artery pressure waveforms: comparison between normal subjects and heart failure patients. *Biomed Mater Eng* 2014;24:271–7.
- Van Bortel LM, Struijker-Boudier HA, Safar ME. Pulse pressure, arterial stiffness, and drug treatment of hypertension. *Hypertension* 2001;38:914–21.
- Kim JW, Park CG, Hong SJ, Park SM, Rha SW, Seo HS, et al. Acute and chronic effects of cigarette smoking on arterial stiffness. *Blood Press* 2009;14:80–5.
- Mahmud A, Feely J. Divergent effect of acute and chronic alcohol on arterial stiffness. *Am J Hypertens* 2002;15:240–3.
- Li F, Yang LC, Shi HY, Liu CY. Differences in photoplethysmography morphological features and feature time series between two opposite emotions: happiness and sadness. *Artery Res* 2017;18:7–13.
- Zheng DC, Murray A. Peripheral arterial volume distensibility: significant differences with age and blood pressure measured using an applied external pressure. *Physiol Meas* 2011;32:499–512.
- Bank AJ, Kaiser DR. Smooth muscle relaxation: effects on arterial compliance, distensibility, elastic modulus, and pulse wave velocity. *Hypertension* 1998;32:356–9.
- Cohn JN, Finkelstein S, McVeigh G, Morgan D, Lemay L, Robinson J, et al. Noninvasive pulse wave analysis for the early detection of vascular disease. *Hypertension* 1995;26:503–8.
- Pirs C, Cigale B, Zazula D. A feasibility study of heartbeat detections from photoplethysmograms with fingers compressed. *Advances in Sensors, Signals, Visualization, Imaging and Simulation*, vol. 6; 2012. p. 47–52.
- Van Bortel LM, Balkestein EJ, van der Heijden-Spek JJ, Vanmolkot FH, Staessen JA, Kragten JA, et al. Non-invasive assessment of local arterial pulse pressure: comparison of applanation tonometry and echo-tracking. *J Hypertens* 2001;19:1037–44.
- Zheng DC, Allen J, Murray A. Non-invasive in vivo assessment of changes in peripheral arterial properties with estimation of arterial volume compliance. *Physiol Meas* 2007;28:1317–27.
- Zheng DC, Murray A. Non-invasive quantification of peripheral arterial volume distensibility and its non-linear relationship with arterial pressure. *J Biomech* 2009;42:1032–7.
- Balmain S, Padmanabhan N, Ferrell WR, Morton JJ, McMurray JJV. Differences in arterial compliance, microvascular function and venous capacitance between patients with heart failure and either preserved or reduced left ventricular systolic function. *Eur J Heart Fail* 2007;9:865–71.
- Bos WJW, Verrij E, Vincent HH, Westerhof BE, Parati G, van Montfrans GA. How to assess mean blood pressure properly at the brachial artery level? *J Hypertens* 2007;25:751–5.
- Zong W, Heldt T, Moody GB, Mark RG. An open-source algorithm to detect onset of arterial blood pressure pulses. *Comput Cardiol* 2003;30:259–62.
- Liu CY, Li Qiao, Clifford Gari D. Evaluation of the accuracy and noise response of an open-source pulse onset detection algorithm on pulsatile waveform databases. *Comput Cardiol* 2016;43:913–6.

23. Pucci G, Battista F, Anastasio F, Sanesi L, Gavish B, Butlin M, et al. Effects of gravity-induced upper-limb blood pressure changes on wave transmission and arterial radial waveform. *J Hypertens* 2016;**34**:1091–8.
24. Gavish B, Gavish L. Simple determination of the systolic-diastolic pressure relationship from blood pressure readings taken at different arm heights. *Blood Press Monit* 2013;**18**:144–50.
25. Gavish B, Gavish L. Blood pressure variation in response to changing arm cuff height cannot be explained solely by the hydrostatic effect. *J Hypertens* 2011;**29**:2099–104.
26. Netea RT, Bijlstra PJ, Lenders JW, Smits P, Thien T. Influence of the arm position on intra-arterial blood pressure measurement. *J Hum Hypertens* 1998;**12**:157–60.
27. Netea RT, Lenders JW, Smits P, Thien T. Both body and arm position significantly influence blood pressure measurement. *J Hum Hypertens* 2003;**17**:459–62.
28. Mitchell PL, Parlin RW, Blackburn H. Effect of vertical displacement of the arm on indirect blood-pressure measurement. *N Engl J Med* 1964;**9**:72–4.
29. Mitchell GF, Tardif JC, Arnold JM, Marchiori G, O'Brien TX, Dunlap ME, et al. Pulsatile hemodynamics in congestive heart failure. *Hypertension* 2001;**38**:1433–9.
30. Arnold JM, Marchiori GE, Imrie JR, Burton GL, Pflugfelder PW, Kostuk WJ. Large artery function in patients with chronic heart failure. Studies of brachial artery diameter and hemodynamics. *Circulation* 1992;**84**:2418–25.
31. Tartière JM, Logeart D, Safar ME, Cohensolal A. Interaction between pulse wave velocity, augmentation index, pulse pressure and left ventricular function in chronic heart failure. *J Hum Hypertens* 2005;**20**:213–9.